



CTD Data RV Heincke HE451-1

Data Processing Report

Contents

1	Introduction	1
2	Workflow	1
3	Cruise details	3
4	Sensor Layout	3
5	Processing	3
6	Results	5

Contact:

Gerd Rohardt

Alfred-Wegener-Institute

Am Handelshafen 12, D-27570 Bremerhaven, GERMANY

Mail: info@awi.de

Processing Agency:

FIELAX

Schleusenstr. 14, D-27568 Bremerhaven, GERMANY

Mail: info@fielax.de

Ref.: CTD-HE451-1-report.pdf	Vers.: 1	Date: 2016/04/07	Status: final
------------------------------	----------	------------------	---------------



1 Introduction

This report describes the processing of CTD raw data acquired by Seabird SBE 911plus CTD on board RV Heincke during expedition HE451-1.

2 Workflow

The different steps of processing and validation are visualized in Figure 1. The CTD raw data are delivered from Gerd Rohardt (AWI). The station book of the RV Heincke cruise is extracted from the DAVIS SHIP data base (https://dship.awi.de). The first CTD station and cast is processed manually in SBE Data Processing to configure the *.psa Seabird routines Data Conversion, Wild Edit, Bottle Summary, Split, Translate, Cell Thermal Mass, Loop Edit and Bin Average. The Seabird routines are then run in a batch job CTDjob in ManageCTD to process the complete CTD data set. The downcast of each CTD station/cast is used for further processing. In CTDjob the start record and the lowest altimeter point of the downcast is selected. With the *Utilities* → *Dship Ebook* function of ManageCTD the DAVIS SHIP station book extraction is used for getting the header information of all CTD stations/casts of the cruise. ManageCTD *Utilities* \rightarrow *Find Profile* function compares station times of the header with the entries in the station book to find out the correct naming of the stations and casts. In CTDheader in ManageCTD the header information of each CTD station/cast is displayed, controlled and corrected if necessary. CTDdespike in ManageCTD is used for a visual check of the data and to erase/interpolate spikes in the data if necessary. Additionally, a sensor pair (Temp1/Sal1 or Temp2/Sal2) is chosen for each station/cast of the RV Heincke cruise in CTDdespike.

ManageCTD *Utilities* \rightarrow *CheckDoubleSensors* controls the quality of temperature and conductivity sensors. For this purpose outliers of too high sensor pair differences could be removed. The data is then converted to spreadsheet format with dsp2odv for visualization of the data in Ocean Data View (ODV). The second visual inspection of the CTD data allows a comparison with data from other CTD casts from close-by stations to verify the oxygen sensor data. Therefore, potential reference cruise data is downloaded from PANGAEA (http://www.PANGAEA.de). The reference data is converted to *.mat format. In the ManageCTD Final Processing the CTD data is displayed together with the reference data. Bad data points, sensors or casts are interpolated or erased from the data set and filters are applied if necessary. The processed CTD data are written to text files and imported to PANGAEA (http://www.PANGAEA.de) for publication.



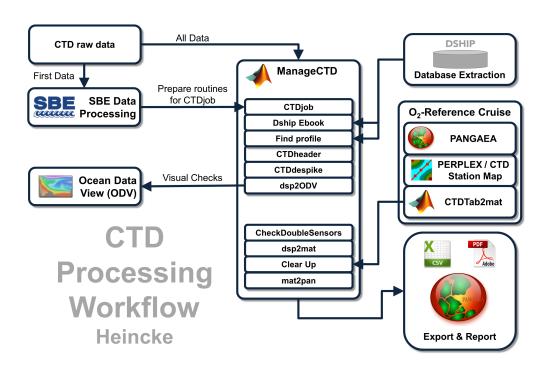


Figure 1: CTD data Processing Workflow



3 Cruise details

Vessel name RV Heincke Cruise name HE451-1

Cruise start 11.09.2015 Tromsø

Cruise end 29.09.2015 Longyearbyen

Cruise duration 19 days
No. of CTD casts 15

4 Sensor Layout

This chapter describes the CTD sensors mounted during this cruise: SBE 911plus CTD (SN: 1015), SBE Instrument Configuration Version 7.23.0.1.

ID	Sensor Name	Serial No.	Calibration Date
55	TemperatureSensor	5354	21-Jan-12
3	ConductivitySensor	2470	15-Nov-13
45	PressureSensor	1015	05-Oct-10
55	TemperatureSensor	5375	21-Jan-12
3	ConductivitySensor	3810	08-Feb-12
0	AltimeterSensor	46466	23-Mar-09
71	WET_LabsCStar	1348DR	13-Oct-2010
20	FluoroWetlabECO_AFL_FL_Sensor	1346	26-Feb-2009
38	OxygenSensor	1597	19-Jun-12

5 Processing

Details of processing procedures and processing parameters are described in *CTD Processing Log-book of RV Heincke* (hdl:10013/epic.47427).

Density Inversions and Manual Validation

Obvius outliers were removed manually. For the visual check density inversions > 0.005 kg/m^3 and > 0.01 kg/m^3 were flagged differently for display but removed automatically. Decisions whether the flagged values were manually removed or not are based on the description in *CTD Processing Logbook of RV Heincke* (hdl:10013/epic.47427).



Sensor Differences

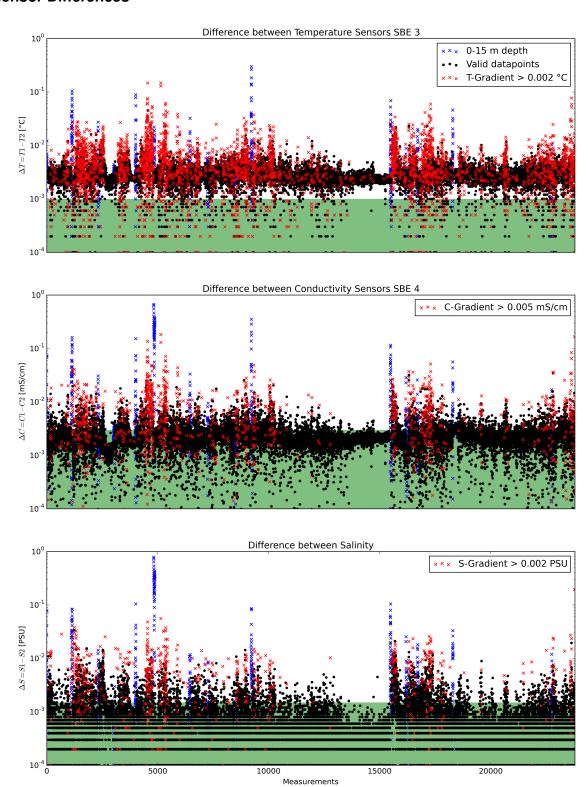


Figure 2: Data accuracy of sensor pairs HE451-1



6 Results

A complete processing overview for each sensor at each station is summarized in the table in the Appendix (Figure 3).

Double Sensor Check

In Figure 2, the absolute residuals between the two sensorpairs are shown for the measured parameters *Temperature* and *Conductivity* and the derived parameter *Salinity*. Measurements in shallow water depths < 15 m (blue crosses) and gradients between two datapoints exceeding a defined threshold (red crosses) were omitted for accuracy calculation.

	Accuracy	Measurements re-	Remaining measure-				
		moved	ments				
Parameter	given by manufacturer	Surface 0-15m + gradi-	within accuracy specifi-				
		ent filter	cations				
Temperature	$\pm 0.001^{\circ}C$	18.71%	3.42%				
Conductivity	$\pm 0.003mS/cm$	8.51%	83.17%				
Salinity	$\pm 0.0015 PSU$	6.25%	87.68%				

Comments

- 15 CTD/RO "on ground" entries in DShip station book
- 15 CTD raw data sets delivered
- 15 CTD casts processed and uploaded
- of these 15 processed CTD casts:
 - 4 oxygen profiles deleted (spiky and not matching to reference casts)
 - 1043 data points interpolated
 - 20 data points erased



Result files

Text File (HE451-1_phys_oce.tab):

The format is a plain text (tab-delimited values) file.

Column separator	Tabulator "\t"
Column 1	Event label
Column 2	Date/Time of event
Column 3	Latitude of event
Column 4	Longitude of event
Column 5	Elevation of event
Column 6	DEPTH, water
Column 7	Pressure, water
Column 8	Temperature, water
Column 9	Conductivity
Column 10	Salinity
Column 11	Temperature, water, potential
Column 12	Density, sigma-theta (0)
Column 13	Oxygen
Column 14	Oxygen, saturation
Column 15	Attenuation, optical beam transmission
Column 16	Fluorometer
Column 17	Number of observations

Processing Report (CTD-HE451-1-report.pdf):

This PDF document.



		oxygen			oxygen			oxygen		no btl file; oxygen offset	n upper 20 m in range	20-250m	ost 0.0									oxygen		
	Comments	no btl file; oxygen	deleted	no btl file	no btl file; oxygen	deleted	no btl file	no btl file; oxygen	deleted	no btl file;	in upper 2	+1.5/-0.5, 20-250m	offset almost 0.0	no btl file	no btl file	no btl file	no btl file	no btl file	no btl file	no btl file	no btl file	no btl file; oxygen	deleted	
e e	Offset			~-0.4			~-0.6						~0.0	~-0.5	~-0.4	~0.5	~0.3	~0.2	~0.0	~0.0	~0.1			
Oxygen reference	dist. (km)		5.81	17.59		52.11	98.34		130.2				14.32	80.0	6.71	3.76	0.29	48.41	4.89	7.14	60.17		2.24	
Oxygen	cruise/sss-cc dist. (km) Offset		0 HE333/27-1 45.81	HE333/19-1 217.59		HE333/19-1 252.11	HE333/17-1 198.34		0 HE333/17-1 1				0 HE333/59-1 214.32	HE333/65-1 90.08	HE333/65-1 86.71	HE333/59-1 83.76	HE333/59-1 50.29	HE333/59-1 4	HE333/65-1 44.89	HE333/65-1 37.14	HE333/59-1 (0 HE333/17-1 72.24	
ete	_		0	0		0	0		0				0	0	0	0	0	0	20	0	0		0	20
complete	interp erased		24	25		42	61		32				110	99	275	9	15	110	161	32	31		4	1043
>																			4					4
Oxy	interp erased			5			12						22	6	55	13	3	20	32	9	9			183
'n																			4					4
Fluor	interp erased		9	5		10	12		8				22	6	55	13	3	20	32	9	9		1	208
ns	erased																		4					4
Trans	interp erased		9	5		10	12		8				22	6	22	13	3	20	32	9	9		1	208
Sal	erased																		4					4
Š	interp erased		9	9		12	13		8				22	18	22	13	8	08	88	8	4		1	234
Temp	interp erased																		4					4
Te	interp		9	2		10	12		8				22	11	22	13	3	20	32	9	9		1	210
Sensor	pair		1	1		2	1		1				2	2	2	1	1	2	2	7	2		2	
ie	HE451_		001-1.*	*:7-100		003-1.*	04-1.*		005-1.*				006-1.*	07-1.*	08-1.*	*.1-600	010-1.*	011-1.*	*1-210	013-1.*	0014-1.*		015-1.*	
Depth File	[m]			203.9		175.3	343.4		168.9				252.3	158.4 007-:	1252.3008-	146.4	104.8	325.4	6.288	231.2	255.9		153.6	
Position	Longitude		15° 43.75' E	6.07' E			17° 13.54' E		20° 1.51' E				13° 36.38' E		6° 5.89' E	11° 58.18' E	11° 33.24' E	10° 44.27' E 325.4			11° 38.24' E		16° 31.03' E	
Position	Latitude		0001-1 CTD/RO 13.09.2015 7:46 76° 58.68' N 15° 43.75' E 230.2	15.09.2015 10:05 80° 11.11' N 22°		5:57 80° 30.17' N 22° 0.28' E	6:05 80° 0.55' N 17° 13.54' E 343.4 004-		79° 25.90' N 20° 1.51' E				6:03 80° 26.13' N 13° 36.38' E 252.3	6:03 79° 27.55' N 8° 42.30' E	6:20 79° 7.68' N	8:43 79° 14.41' N 11° 58.18' E 146.4	CTD/RO 23.09.2015 6:23 78° 51.42' N 11° 33.24' E 104.8	8:45 79° 1.11' N	CTD/RO 25.09.2015 6:16 79° 0.18' N 8° 14.86' E	CTD/RO 25.09.2015 15:05 78° 58.16' N 8° 42.46' E	6:23 79° 0.00' N		6:21 78° 35.44' N 16° 31.03' E 153.6 0015-1.*	
_	=		7:46	10:05		5:57			6:30						6:20		6:23		6:16	15:05				
	Date		13.09.2015	15.09.2015		0003-1 CTD/RO 16.09.2015	17.09.2015		18.09.2015				0006-1 CTD/RO 19.09.2015	CTD/RO 20.09.2015	CTD/RO 21.09.2015	CTD/RO 22.09.2015	23.09.2015	CTD/RO 24.09.2015	25.09.2015	25.09.2015	26.09.2015		27.09.2015	
Gear			CTD/RO	CTD/RO		CTD/RO	CTD/RO		CTD/RO				CTD/RO	CTD/RO	CTD/RO	CTD/RO	CTD/RO	CTD/RO	CTD/RO	CTD/RO	CTD/RO		CTD/RO	
Station	HE451/ Abbr.		0001-1	0002-1		0003-1	0004-1		0005-1				0006-1	0007-1	0008-1	1-6000	0010-1	0011-1	0012-1	0013-1	0014-1		0015-1	

Figure 3: CTD data Processing Summary HE451-1 Page 7 of 8



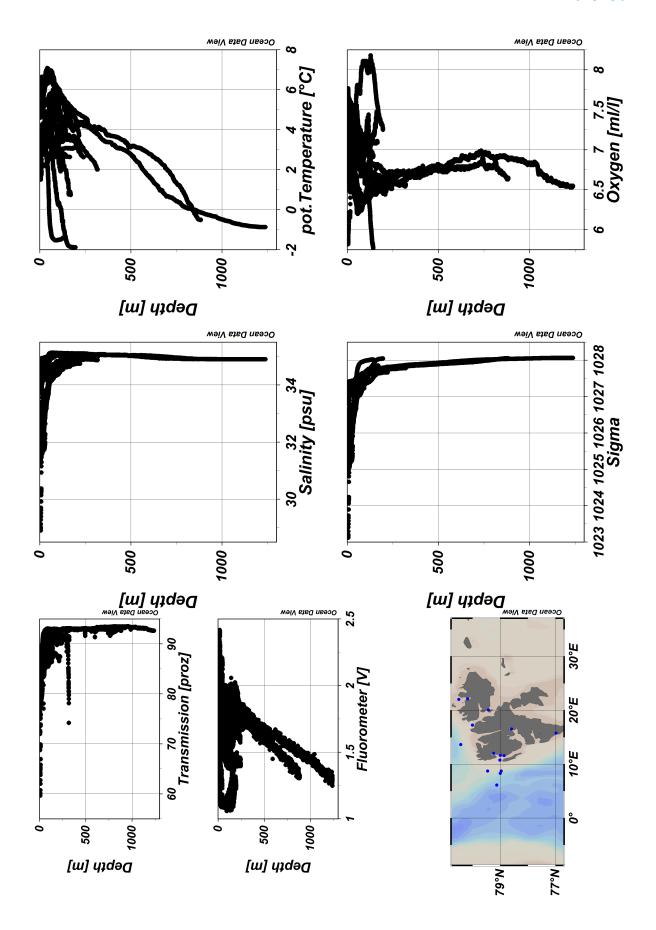


Figure 4: ODV Screenshot of HE451-1 CTD data Page 8 of 8